

इंटरनेट

मानक

Disclosure to Promote the Right To Information

Whereas the Parliament of India has set out to provide a practical regime of right to information for citizens to secure access to information under the control of public authorities, in order to promote transparency and accountability in the working of every public authority, and whereas the attached publication of the Bureau of Indian Standards is of particular interest to the public, particularly disadvantaged communities and those engaged in the pursuit of education and knowledge, the attached public safety standard is made available to promote the timely dissemination of this information in an accurate manner to the public.

“जानने का अधिकार, जीने का अधिकार”

Mazdoor Kisan Shakti Sangathan

“The Right to Information, The Right to Live”

“पुराने को छोड़ नये के तरफ”

Jawaharlal Nehru

“Step Out From the Old to the New”

IS 13360-11-15 (2006): Plastics - Methods of testing, Part 11: Special properties, Section 15: Determination of viscosity using a falling-ball viscometer - inclined-tube method [PCD 12: Plastics]



“ज्ञान से एक नये भारत का निर्माण”

Satyanarayan Gangaram Pitroda

“Invent a New India Using Knowledge”



“ज्ञान एक ऐसा खजाना है जो कभी चुराया नहीं जा सकता है”

Bhartrhari—Nitiśatakam

“Knowledge is such a treasure which cannot be stolen”

BLANK PAGE



भारतीय मानक
प्लास्टिक — परीक्षण पद्धतियाँ

भाग 11 विशेष गुणधर्म

अनुभाग 15 फालिंग-बॉल श्यानतामापी के प्रयोग से श्यानता ज्ञात करना — आनत-ट्यूब पद्धति

Indian Standard

PLASTICS — METHODS OF TESTING

PART 11 SPECIAL PROPERTIES

Section 15 Determination of Viscosity Using a Falling-Ball Viscometer — Inclined-Tube Method

ICS 83.080.01

© BIS 2006

BUREAU OF INDIAN STANDARDS
MANAK BHAVAN, 9 BAHADUR SHAH ZAFAR MARG
NEW DELHI 110002

August 2006

Price Group 3

NATIONAL FOREWORD

This Indian Standard (Part 11/Sec 15) which is identical with ISO 12058-1 : 1997 'Plastics — Determination of viscosity using a falling-ball viscometer — Inclined-tube method' issued by the International Organization for Standardization (ISO) was adopted by the Bureau of Indian Standards on the recommendation of the Plastics Sectional Committee and approval of the Petroleum, Coal and Related Products Division Council.

The text of ISO Standard has been approved as suitable for publication as an Indian Standard without deviations. Certain conventions are, however, not identical to those used in Indian Standards. Attention is particularly drawn to the following:

- a) Wherever the words 'International Standard' appear referring to this standard, they should be read as 'Indian Standard'.
- b) Comma (,) has been used as a decimal marker while in Indian Standards, the current practice is to use a point (.) as the decimal marker.

In this adopted standard, reference appears to the following International Standard for which Indian Standard also exists. The corresponding Indian Standard which is to be substituted in its place is listed below along with its degree of equivalence for the edition indicated:

<i>International Standard</i>	<i>Corresponding Indian Standard</i>	<i>Degree of Equivalence</i>
ISO 2811-1 : 1997 Paints and varnishes — Determination of density — Part 1 : Pyknometer method	IS 101 (Part 1/Sec 7) : 1987 Methods of sampling and test for paints, varnishes and related products: Part 1 Test on liquid paints (general and physical), Section 7 Mass per 10 litres (<i>third revision</i>)	Technically Equivalent

In reporting the results of a test or analysis made in accordance with this standard, if the final value, observed or calculated, is to be rounded off, it shall be done in accordance with IS 2 : 1960 'Rules for rounding off numerical values (*revised*)'.

Indian Standard

PLASTICS — METHODS OF TESTING

PART 11 SPECIAL PROPERTIES

Section 15 Determination of Viscosity Using a Falling-Ball Viscometer — Inclined-Tube Method

1 Scope

This part of ISO 12058 specifies the general principles of a method, using an inclined-tube falling-ball viscometer, for determining the viscosity of polymers and resins in the liquid emulsified or dispersed state. It is intended for application to liquids over a viscosity measurement range of 0,6 mPa·s to 250 000 mPa·s (temperature range – 20 °C to + 120 °C) for which the shear stress and shear rate are proportional, i.e. the viscosity is independent of the shear rate. This ideal behaviour is commonly known as Newtonian behaviour. If a liquid differs significantly from this behaviour, different results may be obtained with the different balls of a falling-ball viscometer or from viscometers with different geometries, such as capillary and rotational viscometers.

2 Normative reference

The following standard contains provisions which, through reference in this text, constitute provisions of this part of ISO 12058. At the time of publication, the edition indicated was valid. All standards are subject to revision, and parties to agreements based on this part of ISO 12058 are encouraged to investigate the possibility of applying the most recent edition of the standard indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 2811-1:—¹⁾, *Paints and varnishes — Determination of density — Part 1: Pyknometer method.*

3 Principle

The viscosity of a liquid is determined by observing the motion of a solid sphere under the influence of gravity in an inclined cylindrical tube filled with the liquid.

4 Measurand and units

Dynamic viscosity, expressed in millipascal seconds (mPa·s).

1) To be published. (Revision of ISO 2811:1974)

5 Measurement range and temperature range

Viscosity-measurement range: 0,6 mPa·s to 250 000 mPa·s
Minimum falling time for ball: 60 s for ball No. 1 ²⁾
50 s for balls 2 to 4
30 s for balls 5 and 6
Temperature range: - 20 °C to + 120 °C

6 Apparatus

6.1 Falling-ball viscometer³⁾ (see figure 1)

The apparatus consists of an inclined measurement tube (falling-ball tube) filled with the liquid under test and made of thermally aged, calibrated, precision borosilicate-glass tubing with a coefficient of linear expansion of $3,3 \times 10^{-6} \text{ }^{\circ}\text{C}^{-1}$, plus six balls of diameter 15,81 mm to 11,0 mm (see table 1), each of balls 1 to 4 having the same coefficient of expansion as the tube itself. To minimize errors, the measurement tube and balls shall be free of flaws.

Table 1 — Balls for use in falling-ball viscometer having a measurement tube with an inside diameter of 15,94 mm ± 0,01 mm

Ball No.	Material	Density, ρ_1 (typical)	Diameter mm	Out-of-roundness mm	Constant K (typical) mPa·s·cm ³ /(g·s)	Dynamic-viscosity measurement range (typical) mPa·s
		g/cm ³				
1	Borosilicate glass	2,4	15,81 ± 0,01	± 0,000 5	0,007	0,6 to 10
2	Borosilicate glass	2,4	15,60 ± 0,05	± 0,000 5	0,09	7 to 130
3	Nickel-iron	8,1	15,60 ± 0,05	± 0,001	0,09	30 to 700
4	Nickel-iron	8,1	15,2 ± 0,1	± 0,001	0,7	200 to 4 800
5	Nickel-iron or steel	7,7 to 8,1	14,0 ± 0,5	± 0,001	7	1 500 to 45 000
6	Steel	7,7 to 7,8	11 ± 1	± 0,002	35	> 7 500

For a given ball, the calibration constant K of the apparatus depends on the internal diameter of the tube. The values given in table 1 apply to a tube 15,94 mm ± 0,01 mm in diameter.

The measurement tube has two circular marks defining the measurement distance to within 100 mm ± 1 mm. The tube is surrounded by a tubular glass jacket for temperature control and fixed to a stand in such a manner that the axis of the tube is inclined at 10° ± 1° to the vertical for measurement purposes⁴⁾. The measurement tube and the glass jacket can be inverted by rotating them together about their mounting point on the stand in order to return the ball to the starting position. The ends of the measurement tube are closed with two plugs, one of which contains a capillary joined to a hollow space. This type of closure prevents unacceptable pressure variations occurring, as well as the entry of air due to temperature fluctuations. The liquid under test is completely surrounded by the jacket and plugs, thus preventing evaporation or the formation of a surface skin. The stand is equipped with a spirit level and feet with levelling screws. A removable thermometer is fitted (see 6.2).

Each viscometer shall have a test certificate, issued by the manufacturer or by a third party, stating the individual apparatus constants. The viscometer shall be recalibrated whenever a new measurement tube or a new ball is used or when considerable demands are placed on the viscometer (e.g. a series of measurements on aggressive liquids).

2) See table 1.
3) The determination of viscosity using an inclined-tube falling-ball viscometer may be carried out using equipment supplied by a number of manufacturers. One example of such an instrument is the Høepler viscometer as described in DIN 53015:1978, *Viscometry; Measurement of viscosity using the Høepler falling-ball viscometer*.
4) Apparatus with an inclination other than 10° is not suitable for use with this part of ISO 12058.

Dimensions in millimetres

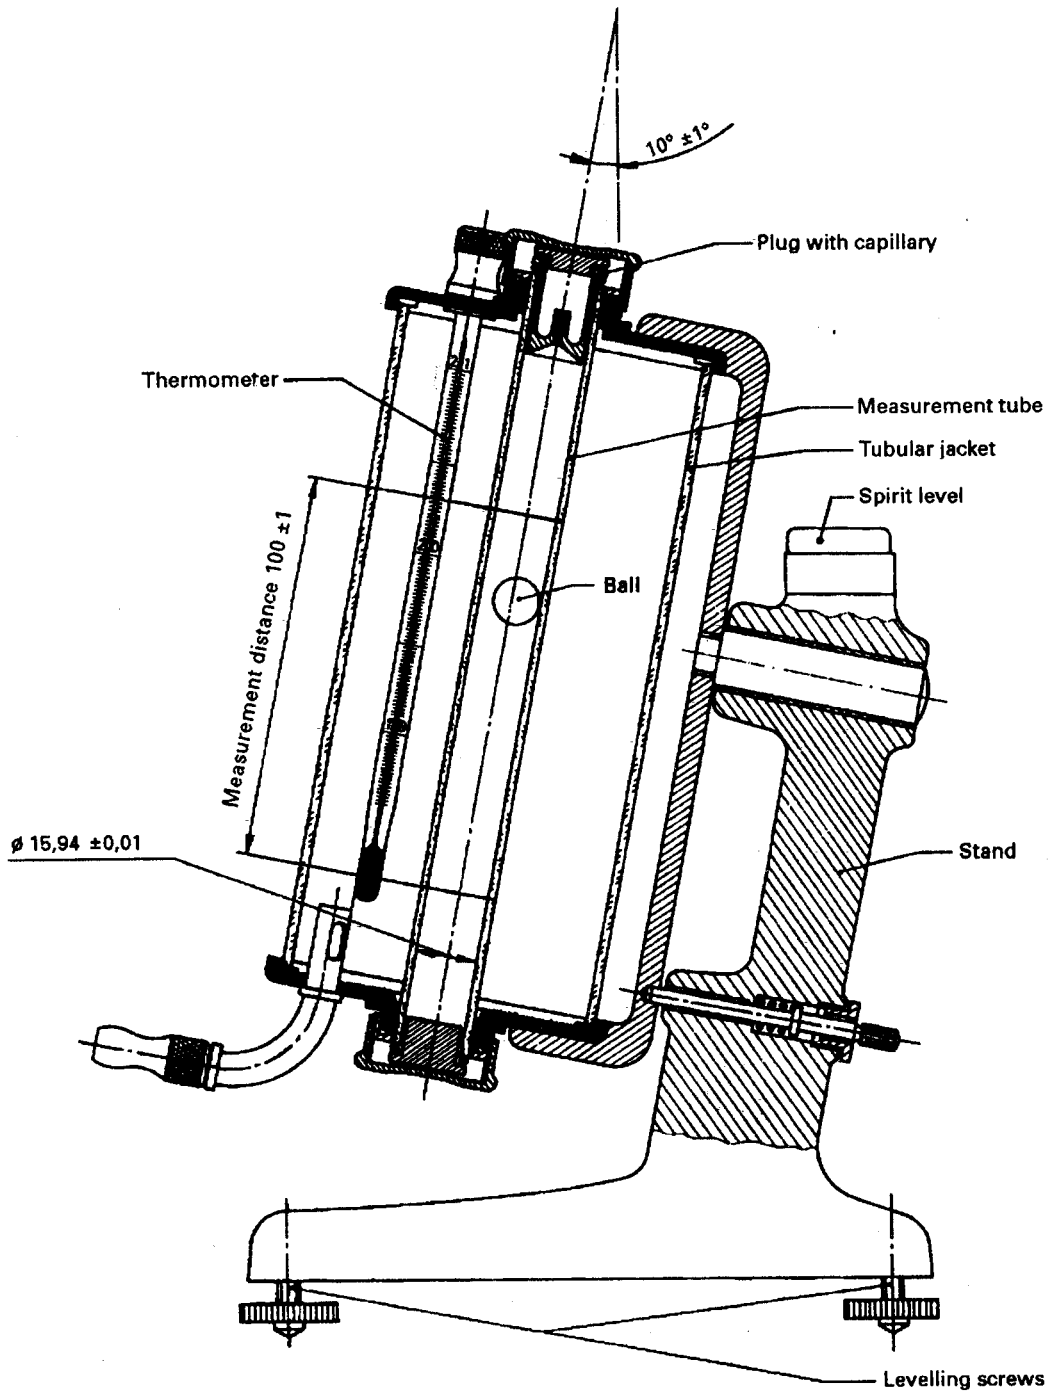


Figure 1 — Typical falling-ball viscometer

6.2 Thermometer

The special thermometer used in the apparatus is placed in the liquid in the thermal jacket. It shall have a scale graduated at intervals of not more than $0,1^\circ\text{C}$. It shall be calibrated totally immersed, and shall be capable of measuring the temperature to $\pm 0,03^\circ\text{C}$. The thermometer reading shall be corrected as indicated in the calibration certificate. The thermometer shall be protected against radiant heat during the measurement.

6.3 Timer

The time taken by the ball to travel the distance between the two circular marks shall be measured using one of the following.

6.3.1 Stopwatch, having a scale interval not greater than 0,1 s. The stop watch shall be compared from time to time with a standard clock accurate to within 15 s in 24 h. It is advisable to use calibrated stopwatches.

6.3.2 Electronic timer, based on frequency counting or comprising synchronous clocks. The frequency used shall be constant to within 10^{-4} of its normal value.

6.3.3 Automatic timer, with the same accuracy as the stopwatch (6.3.1).

6.4 Thermostat

The temperature in the jacket shall be maintained constant, by means of a thermostat, to within at least $\pm 0,03$ °C over the temperature range from 10 °C to 80 °C and to within $\pm 0,05$ °C at temperatures outside this range. Only fluorescent tubes, which radiate little heat, shall be used to illuminate the apparatus.

7 Sampling

Sampling shall be carried out in accordance with the specification or standard for the liquid under test.

8 Procedure

Ensure that all parts of the apparatus coming into contact with the liquid under test are clean⁵⁾ and dry.

Pour the liquid under test into the measurement tube and introduce the ball. Then place the plug with the capillary in the upper end of the measurement tube and screw tight. The ball shall not have any bubbles adhering to it. Maintain the liquid under test at the specified test temperature for at least 15 min⁶⁾. Before each series of measurements, roll the ball along the length of the tube once in order to ensure thorough mixing of the liquid. Then measure the time the ball takes to travel between the two circular marks (see figure 1).

Repeat the measurement at least three times.

If the density of the liquid under test is not known, determine it in accordance with ISO 2811-1.

9 Expression of results

Calculate the dynamic viscosity η , expressed in millipascal seconds, using the following equation:

$$\eta = K(\rho_1 - \rho_2) t$$

where

K is the calibration constant of the instrument (see table 1 and 6.1);

ρ_1 is the density, in grams per cubic centimetre, of the ball (see table 1);

ρ_2 is the density, in grams per cubic centimetre, of the liquid under test;

t is the time, in seconds, for the ball to travel the distance between the two marks.

Take as the result the average, rounded to three significant figures, of the determinations carried out.

5) Usually the tube is cleaned by rinsing it with a suitable solvent.

6) If highly viscous liquids are measured or if the measurement temperature differs by more than about 20 °C from room temperature, equilibration may require significantly longer than 15 min.

10 Precision

To assess the reliability of results, the following principles are used:

Repeatability (same operator, same apparatus, same procedure)

If two results are obtained under repeatability conditions, both results may be regarded as acceptable and in accordance with this part of ISO 12058 if they differ from their mean value by not more than the appropriate limit given in table 2.

Reproducibility (different operators, different apparatus, but same procedure)

If a result is obtained under reproducibility conditions in each of two different laboratories, both results may be regarded as acceptable and in accordance with this part of ISO 12058 if they do not differ from their mean value by more than the appropriate limit given in table 2.

Table 2 — Repeatability and reproducibility limits

Ball No.	Repeatability limit, %	Reproducibility limit, %
1	1,0	2
2 to 4	0,5	1
5	0,7	1,5
6	1,5	3
The values given in this table were established following tests performed in Germany using DIN 53015:1978, <i>Viscometry; Measurement of viscosity using the Hoeppler falling-ball viscometer.</i>		

11 Test report

The test report shall include the following information:

- a) the reference number of this part of ISO 12058;
- b) all details necessary for complete identification the material under test;
- c) the date of sampling;
- d) the test temperature, in degrees Celsius;
- e) the average dynamic viscosity, in millipascal seconds;
- f) any deviations from the procedure specified;
- g) any unusual features noted during the determination;
- h) the date of the test;
- i) the name and signature of the person responsible for the determination.

Bureau of Indian Standards

BIS is a statutory institution established under the *Bureau of Indian Standards Act, 1986* to promote harmonious development of the activities of standardization, marking and quality certification of goods and attending to connected matters in the country.

Copyright

BIS has the copyright of all its publications. No part of these publications may be reproduced in any form without the prior permission in writing of BIS. This does not preclude the free use, in the course of implementing the standard, of necessary details, such as symbols and sizes, type or grade designations. Enquiries relating to copyright be addressed to the Director (Publications), BIS.

Review of Indian Standards

Amendments are issued to standards as the need arises on the basis of comments. Standards are also reviewed periodically; a standard along with amendments is reaffirmed when such review indicates that no changes are needed; if the review indicates that changes are needed, it is taken up for revision. Users of Indian Standards should ascertain that they are in possession of the latest amendments or edition by referring to the latest issue of 'BIS Catalogue' and 'Standards : Monthly Additions'.

This Indian Standard has been developed from Doc : PCD 12 (1806).

Amendments Issued Since Publication

Amend No.	Date of Issue	Text Affected

BUREAU OF INDIAN STANDARDS

Headquarters:

Manak Bhavan, 9 Bahadur Shah Zafar Marg, New Delhi 110 002
Telephones : 2323 0131, 2323 3375, 2323 9402 Website : www.bis.org.in

Regional Offices :

	Telephones
Central : Manak Bhavan, 9 Bahadur Shah Zafar Marg NEW DELHI 110 002	{ 2323 7617 2323 3841
Eastern : 1/14 C. I. T. Scheme VII M, V. I. P. Road, Kankurgachi KOLKATA 700 054	{ 2337 8499, 2337 8561 2337 8626, 2337 9120
Northern : SCO 335-336, Sector 34-A, CHANDIGARH 160 022	{ 260 3843 260 9285
Southern : C. I. T. Campus, IV Cross Road, CHENNAI 600 113	{ 2254 1216, 2254 1442 2254 2519, 2254 2315
Western : Manakalaya, E9 MIDC, Marol, Andheri (East) MUMBAI 400 093	{ 2832 9295, 2832 7858 2832 7891, 2832 7892

Branches: AHMEDABAD. BANGALORE. BHOPAL. BHUBANESHWAR. COIMBATORE.
FARIDABAD. GHAZIABAD. GUWAHATI. HYDERABAD. JAIPUR. KANPUR.
LUCKNOW. NAGPUR. PARWANOO. PATNA. PUNE. RAJKOT.
THIRUVANANTHAPURAM. VISAKHAPATNAM.